

AD-A073 759

ARMY ARMAMENT RESEARCH AND DEVELOPMENT COMMAND WATER--ETC F/G 14/2  
AUTOMATIC ULTRASONIC DETECTION AND MEASUREMENT OF CRACKS IN CAN--ETC(U)  
APR 79 D C WINTERS

UNCLASSIFIED

ARLCB-TR-79003

SRIF-AD-F440 036

NI

| OF |  
AD  
A073 759



END  
DATE  
FILMED  
10-79  
DDC



AD A 073759

**LEVEL**

AD-E440 036


TECHNICAL REPORT ARLCB-TR-79003

12

**AUTOMATIC ULTRASONIC DETECTION AND MEASUREMENT  
OF CRACKS IN CANNON**

D. C. Winters

April 1979

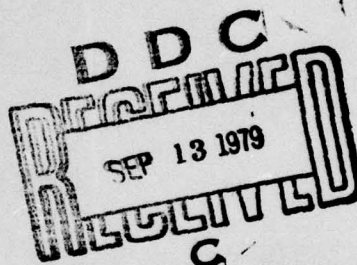

**US ARMY ARMAMENT RESEARCH AND DEVELOPMENT COMMAND  
LARGE CALIBER WEAPON SYSTEMS LABORATORY  
BENET WEAPONS LABORATORY  
WATERVLIET, N. Y. 12189**

AMCMS No. 32910673190

DA Project No. 6787319

PRON No. 1A827046GGGG

DDC FILE COPY

APPROVED FOR PUBLIC RELEASE; DISTRIBUTION UNLIMITED

79 08 15 027

#### DISCLAIMER

The findings in this report are not to be construed as an official Department of the Army position unless so designated by other authorized documents.

The use of trade name(s) and/or manufacturer(s) does not constitute an official indorsement or approval.

#### DISPOSITION

Destroy this report when it is no longer needed. Do not return it to the originator.



SECURITY CLASSIFICATION OF THIS PAGE (When Data Entered)

REPORT DOCUMENTATION PAGE		READ INSTRUCTIONS BEFORE COMPLETING FORM
1. REPORT NUMBER ARLCB-TR-79003	2. GOVT ACCESSION NO.	3. RECIPIENT'S CATALOG NUMBER
4. TITLE (and Subtitle)  Automatic Ultrasonic Detection and Measurement of Cracks in Cannon		5. TYPE OF REPORT & PERIOD COVERED
		6. PERFORMING ORG. REPORT NUMBER
7. AUTHOR(s)  D. C. Winters		8. CONTRACT OR GRANT NUMBER(s)
9. PERFORMING ORGANIZATION NAME AND ADDRESS Benet Weapons Laboratory Watervliet Arsenal, Watervliet, N.Y. 12189 DRDAR-LCB-TL		10. PROGRAM ELEMENT, PROJECT, TASK AREA & WORK UNIT NUMBERS AMENS No. 32910673190 DA Project No. 6797319 PRON No. 1A827046GGGG
11. CONTROLLING OFFICE NAME AND ADDRESS US Army Armament Research and Development Command Large Caliber Weapons Systems Laboratory Dover, New Jersey 07801		12. REPORT DATE April 1979
14. MONITORING AGENCY NAME & ADDRESS (if different from Controlling Office)		13. NUMBER OF PAGES 18
		15. SECURITY CLASS. (of this report)  UNCLASSIFIED
		15a. DECLASSIFICATION/DOWNGRADING SCHEDULE
16. DISTRIBUTION STATEMENT (of this Report)  Approved for public release; distribution unlimited.		
17. DISTRIBUTION STATEMENT (of the abstract entered in Block 20, if different from Report)		
18. SUPPLEMENTARY NOTES  Presented at the 27th Defense Conference on Nondestructive Testing, Yuma, Arizona, Oct. 1978		
19. KEY WORDS (Continue on reverse side if necessary and identify by block number)  Automatic Cracks End-On Ultrasonic		
20. ABSTRACT (Continue on reverse side if necessary and identify by block number)  <u>ABSTRACT</u>  The "end-on" ultrasonic crack measurement technique has been refined and perfected to provide reliable automatic sensing and read out of the maximum crack depth and its location for each crack encountered as the probe moves in		

(Block No. 20 continued)

helical path down the cannon tube. A mechanical scanning machine has been constructed and tested which inspects full length 105 millimeter cannon. An ultrasonic flaw detector senses, measures and continuously reads out the distance from the outside surface to the crack tip or bore surface. Digital logic circuits evaluate successive measurements and determine the maximum crack depth reading. Encoders determine the location of each maximum crack depth reading. This data is transferred to a data acquisition system.

Accession For		<input checked="checked" type="checkbox"/>
NTIS GRA&I		<input type="checkbox"/>
DDC TAB		<input type="checkbox"/>
Unannounced		<input type="checkbox"/>
Justification		<input type="checkbox"/>
By _____		
Distribution/		
Availability Codes		
Dist	Avail and/or	
A	special	

## TABLE OF CONTENTS

	<u>Page</u>
END-ON TECHNIQUE	1
AUTOMATIC SYSTEM	4
MECHANICAL SCANNING SYSTEM	5
ULTRASONIC SYSTEM	9
SYSTEM PERFORMANCE	12
DATA ACQUISITION AND ANALYSIS SYSTEM	13
CONCLUSIONS	14

## ILLUSTRATIONS

1. a. SCHEMATIC OF PROBE-CRACK ORIENTATION ; b. SCHEMATIC OF FLAW DETECTOR PRESENTATION	1
2. FATIGUE DEMARCATION, FRACTURE SURFACE SPECIMEN 58805	2
3. CRACK DEPTH (ULTRASONIC) VS. CRACK DEPTH (VISUAL)	3
4. AUTOMATED ULTRASONIC FATIGUE CRACK MAP 8 INCH HOWITZER M2A2	5
5. ULTRASONIC SCANNING SYSTEM	6
6. CONTROL PANEL AND FLAW DETECTOR	7
7. VIEW OF MOVEABLE PROBE HEAD	8
8. ULTRASONIC FLAW DETECTOR AND DIGITAL LOGIC SUBSYSTEM	11



## END-ON TECHNIQUE

At Benet Weapons Laboratory we have developed and refined a technique for accurate end-on measurement of crack depth using a normal beam ultrasonic probe working with an ultrasonic flaw detector. The probe is coupled to the surface of the cylinder with oil, and the flat probe face rests on the curved cylinder wall as in Figure 1. The ultrasonic signal is reflected from the inside diameter and from the tip of the crack. The difference between the leading edges of these two reflections is the crack depth.


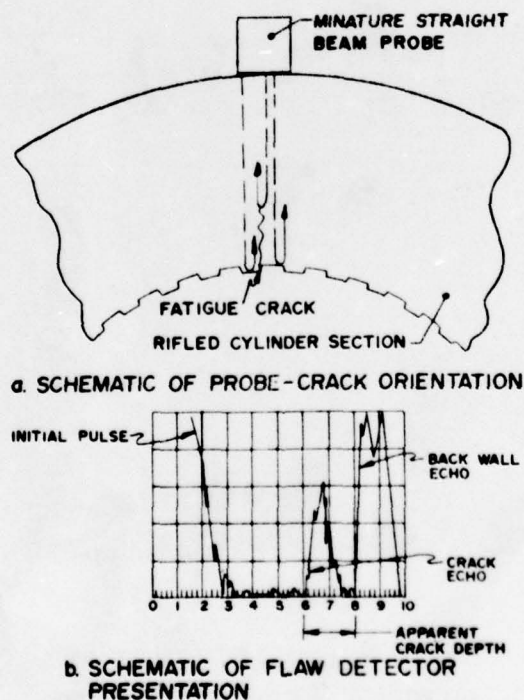


Figure 1

The ultrasonic signal reflects from the small jagged facets at or near the crack tip. Figure 2 shows a fracture surface from a cylinder that has been fatigue cycled at pressure until the crack has grown to 0.08 inch. Many cycles at half pressure have produced the first bench mark. As fatigue cycling has continued further crack growth has occurred. Bench marks have been induced at 0.02 inch, 0.27 inch, 0.30 inch, etc. When the cylinder has failed by fracturing through the wall, it has been wedged open to expose the fatigue crack fracture surface. Visual measurements are then compared to the interim ultrasonic measurements.

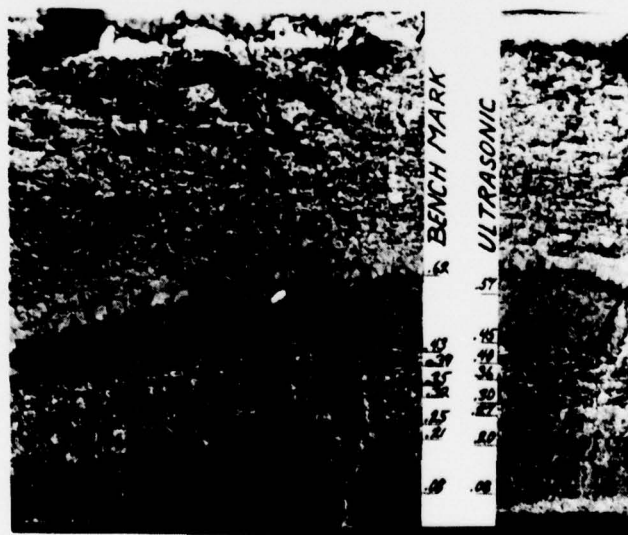

**FATIGUE DEMARCATION, FRACTURE  
SURFACE SPECIMEN 58805**

Figure 2



Figure 3 plots the ultrasonic measurement accuracy as determined on specimen 58805 and three other cylinders. The accuracy of measurement is  $\pm 0.03$  inches. Using this technique it is possible to pick up an initial crack at 0.02 inch but more reliably at 0.05 to 0.08 inches.

In order to get a usable signal reflection from the crack tip the flaw detector gain must be 50 db greater than that gain which will bring the back wall signal to mid-screen on the flaw detector.

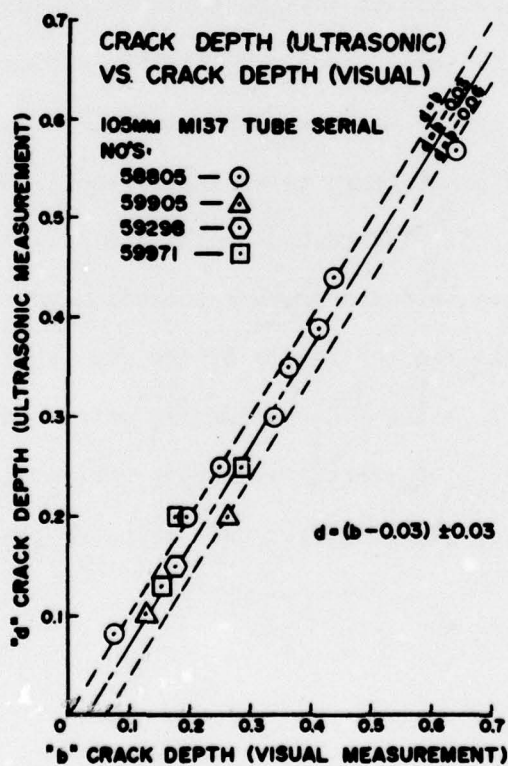


Figure 3

#### AUTOMATIC SYSTEM

It takes several thousand cycles to initiate cracks in gun tubes during fatigue tests. These cracks initiate and grow in the region near the origin of rifling. This whole area is searched about every 500 cycles. There may be only one or two cracks at initiation increasing to a large number such as shown in the crack map of Figure 4 after many sets of cycles. Since it isn't known at the beginning which crack will fail, and since the profile of the crack is important to the study and prediction of fatigue failure, all data, for each 500 cycle scan, is acquired and stored. To do this automatically, an ultrasonic scanning system has been implemented. This system can also inspect cannon after manufacture to evaluate cracks found by magnetic particle inspection. It will record depths and location accurately and this data can then be compared to automatic magnetic particle inspection data taken from the inside of the gun tube. Accurate location information both inside and outside prevents random inclusion signals in the vicinity of cracks from being interpreted as cracks with depth. This will permit better evaluation of gun tubes and less rejects.

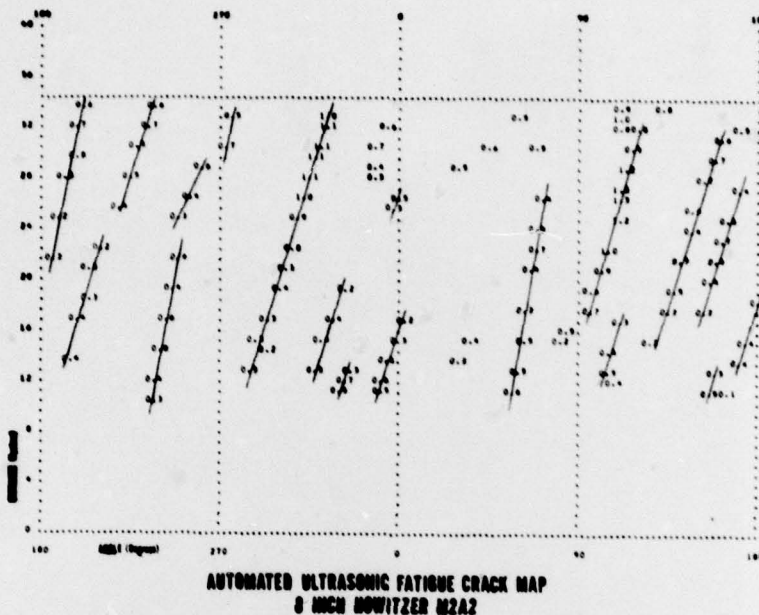


Figure 4

#### MECHANICAL SCANNING SYSTEM

A mechanical scanning machine has been designed and constructed for Benet Weapons Laboratory by the Tektran Division of Arcair Company (Figure 5). It will hold any of three full size gun tubes, the 105 mm M68, the 105 mm M137, or the 105 mm XM205. The heaviest weighs 1660 pounds and is 17.5 feet long.

A stepping motor rotates the gun on adjustable rollers at speeds from 2 to 60 rpm. A second motor moves the ultrasonic inspection probe along the gun at speeds from 0.5 to 15 inches per minute. A full inspection can be completed in fifteen minutes.



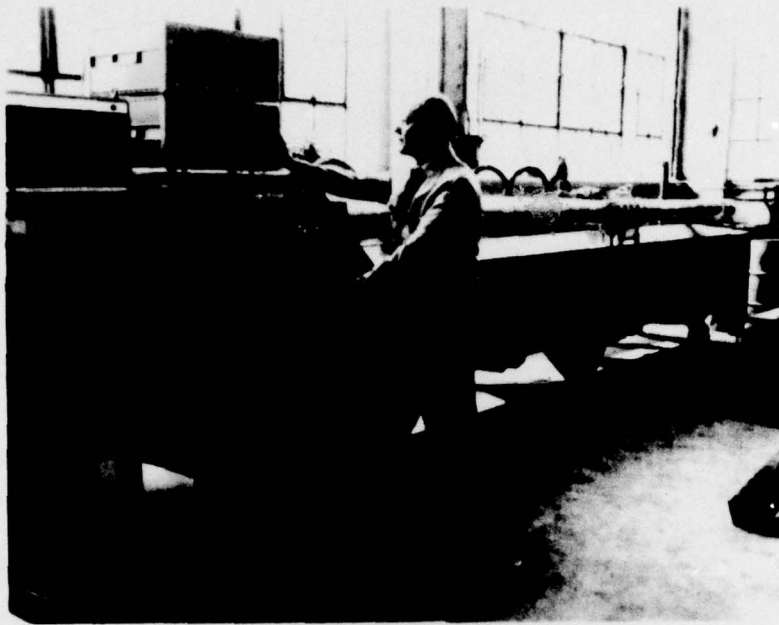


Figure 5

The control panel (Figure 6) has power and speed controls. It has a "home" button for accurately setting the search start position for both rotation and longitudinal position. When the head is returned to this position the position registers in the logic circuit chassis are zeroed. It has a control for the couplant circulator pump. There is a large emergency off knob.

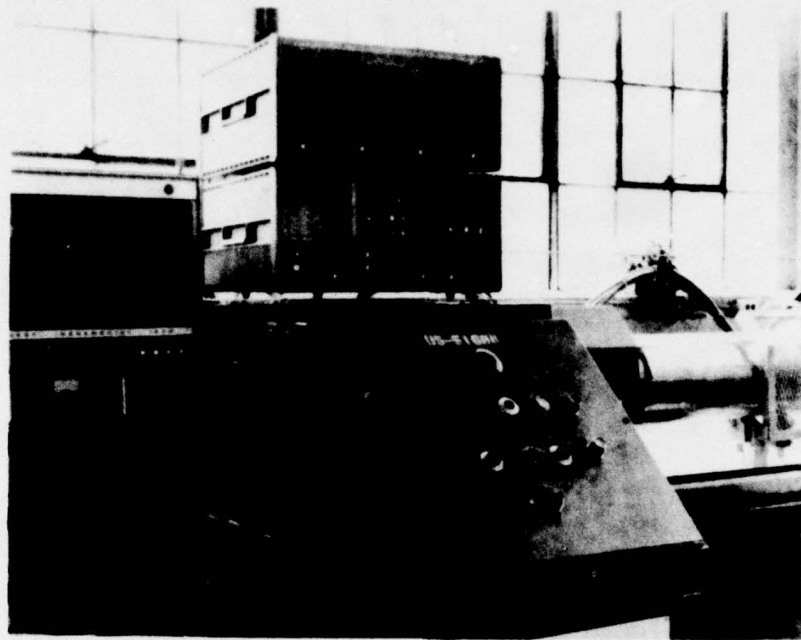


Figure 6

The search head assembly shown in Figure 7 is held against the gun by air pressure. The equipment requires a standard shop supply air line and fitting. The ultrasonic probe is held in a fixture that has roller wheels in contact with the gun. A thin film of oil is pumped into this search head and emerges under the probe. The oil is caught in a full length catch tank. It is then filtered and recirculated. Cams along the back of the tank cause the air supply to the carriage to be activated to move the search head away from the gun until it has passed irregular shapes or threads or sharp tapers on the gun barrel. The next cam moves the head back against the gun.



The whole assembly is mounted on wheels to allow for some portability. Once in position, the leveling jacks are used to level the system.

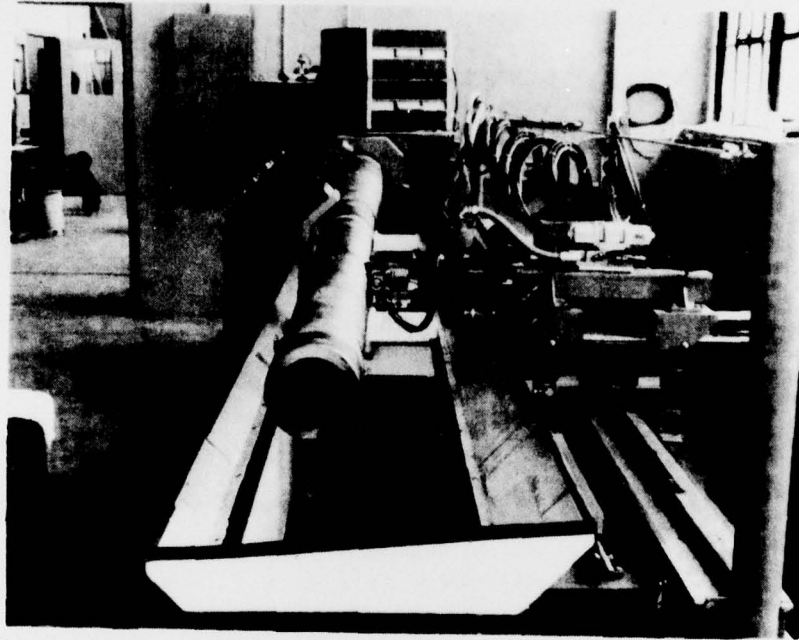


Figure 7

There are two incremental encoders to record the position of the search head relative to a key fixture on the gun, such as a locking slot on the M68. The encoder for rotation is accurate to  $1^\circ$ . It is connected to the gearing driving the chuck and locating dog. The horizontal position encoder is accurate to 0.1 inch. It is driven from the stepping motor which moves the carriage the length of the gun by means of a rack and pinion gear arrangement.

The stepping motors have proven troublesome due to their large voltage pulses which get into the grounding system. Due to a ground loop which couldn't be eliminated they were picked up in the high gain preamplifier stage and appeared in the output as false indication of flaws. The problem was eliminated by synchronizing the flaw detector timing to the stepping motors.

#### ULTRASONIC SYSTEM

A preamplifier is mounted on the probe carriage and gets its power from the main Immerscope flaw detector. Its function is to transform the high impedance of the transducer to the low impedance of the twenty five feet of coaxial cable connecting the preamp to the Immerscope. It is a grounded single ended input amplifier. Stepping motor pulses arriving on the iron frame of the system introduce a ground loop voltage at the transducer case ground. It would require a three wire ungrounded transducer whose return line is connected to the preamp input and which in turn is grounded back at the flaw detector to eliminate this loop. This will require a mechanically modified transducer and cabling, and a redesign of the probe head, since the ground connection is used to physically mount the transducer to the head.

The use of a preamplifier with the flaw detector results in very high gain and a high signal-to-noise ratio. It allows the very small crack signal from the rejected cannon flaw to be displayed almost full scale on the flaw detector screen. Manual measurements that are made

with a Krautkramer USIP11 flaw detector produce very small signals that are barely visible on the screen.

A Tektran Immerscope II is used in this system. It includes the standard SW-25 sweep circuit and the PR-17 Pulser-Receiver unit. An FG/FDC-10 flaw gate and flaw depth circuit module provides distance to crack tip measurements accurate to a hundredth of an inch. Its circuits are configured to provide the depth of the first indication in the gate whose amplitude is greater than 20% of screen height.

Flaw depth data from the Immerscope is continuously fed into the logic circuits at the flaw detector repetition rate. These circuits are located in the C-chassis shown mounted above the flaw detector in Figure 8. This data is continuously subtracted from the wall thickness. The difference is the actual crack depth. As the probe travels over the cannon surface the crack depth numbers change. They get larger as the probe gets more directly over the crack tip and then get smaller as the probe travels on past the directly over position. The logic circuits operate on the changing crack depth readings. The depth numbers are stored in two registers. Register B is the previous reading. Register A is the present reading. If A continues to be larger than B nothing happens. When A becomes smaller than B for the first time that depth reading is transferred to an output register. At this time the position of the probe with respect to the cannon is also transferred to the output registers. This data is then held until it is checked.



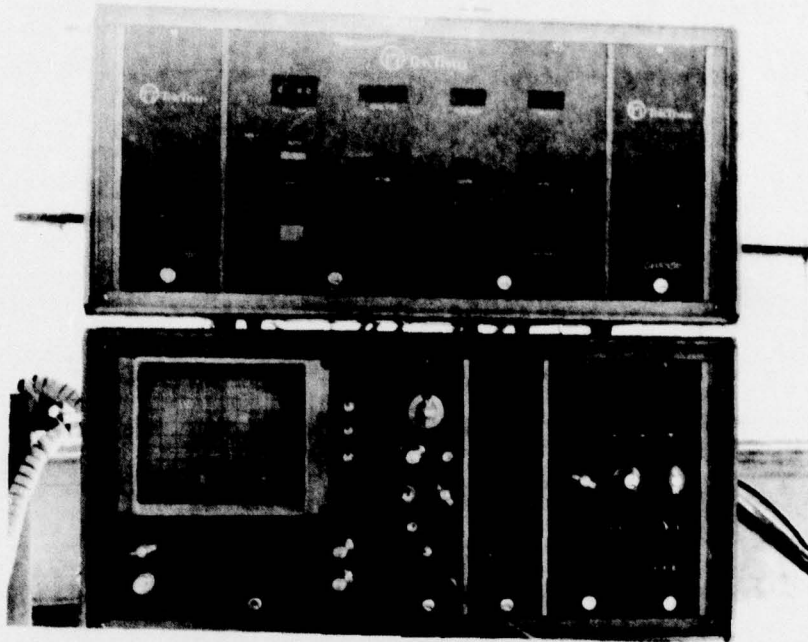


Figure 8

The logic looks for a selected number of A less than B readings up to a maximum of 256. Previous experience has shown that surface noise, intermittent couplant supply, and other factors can cause false maximum readings. If another A greater than B reading occurs before the selected number of checks are finished the logic circuits are reset, a new maximum is found and new depth and position data replace the old. Then another set of checks take place. If no A greater than B reading occurs this time, the new depth and position data replaces the old in the output registers. The new data is not yet sent to the data acquisition system. It must wait for a selected number of degrees of rotation of the cannon. The number can be from

0 to 99 degrees. This is done by counting output pulses from the incremental encoder that encodes rotation position. The number of degrees of hold off can be optimized with respect to the flaw detector repetition rate and the cannon rotation speed. When these checks are concluded a "read out" pulse is generated and the correct updated data is transferred to the data acquisition system. The logic system registers are then reset and ready for the next crack reading.

The position of the probe with respect to the cannon is continuously updated on up-down counters located in the C-chassis. The encoders cause these counters to be incremented or decremented depending on the direction of motion. Position data is transferred from these counters to the output registers when the comparator indicates a maximum.

#### SYSTEM PERFORMANCE

The complete system is now in operation. It has been checked out on a 105 mm M68 cannon that has a defect in it. The defect is an inch long and 0.050 inches deep. During the scanning system acceptance test a plot has been made of the gun along the 0.8 inch thick section of the last 6 feet of the muzzle end which contains the flaw. The scanner hit this flaw three times. It also showed a second flaw a few inches away from the first. Both of these had been seen with black light magnetic particle inspection. The specifications require the system to detect and measure a 0.1" deep crack. The performance exceeds the specs.



The system measures 0.03 inch on the flaw rather than 0.05. This is due to the measurement gate setting being kept about 0.02 inch from the inside diameter signal to avoid false readings on the inside diameter. This offset appears inevitable if data is to be restricted only to flaws.

A present limitation on the use of the scanning system for inspecting full length cannon is the requirement that when the wall thickness changes the new thickness must be measured ultrasonically and manually inserted by means of thumb wheel switches. The gates must also be manually readjusted for this new setting. This limitation can be overcome by having this data stored in a computer memory, along with the appropriate gate settings, and then inserted at the proper time by signals from the length encoder.

#### DATA ACQUISITION AND ANALYSIS SYSTEM

A Digital Equipment Corporation DECLA B11L34-VE data acquisition system is now on order. This will replace our present incremental tape based system which has been used to check out the Tektran equipment. Data will be stored on a removable disk subsystem. It is proposed that for fatigue measurements on field cannon a disk will stay with the gun and at each inspection a new batch of data will be added to the disk.

The data acquisition system is based on a PDP11/34 minicomputer with 32K words of MOS memory and a capability for using Fortran IV language. Programs have been written for the laboratory IBM 360 computer which select the maximum crack from the data on a cannon.

They will be adapted to the PDP11/34. Programs will be written that predict remaining fatigue life from the crack growth curves using fracture toughness criteria. A DECWRITER 11 will be a part of this system and will produce crack "maps" similar to Figure 4 for each set of crack data taken.

#### CONCLUSIONS

The "end on" ultrasonic crack measurement technique is utilized to both read the crack depth and determine its location.

The prototype mechanical scanning system has been tested and performs correctly.

The ultrasonic preamplifier and flaw detector are able to measure a crack 0.050" deep, which exceeds the specification.

The digital logic circuitry for determining the true maximum crack depth and location works correctly.

# WATERVLIET ARSENAL INTERNAL DISTRIBUTION LIST

	<u>NO. OF COPIES</u>
COMMANDER	1
DIRECTOR, BENET WEAPONS LABORATORY	1
CHIEF, DEVELOPMENT ENGINEERING BRANCH	1
ATTN: DRDAR-LCB-DA	1
-DM	1
-DP	1
-DR	1
-DS	1
-DC	1
CHIEF, ENGINEERING SUPPORT BRANCH	1
CHIEF, RESEARCH BRANCH	2
ATTN: DRDAR-LCB-RA	1
-RC	1
-RM	1
-RP	1
TECHNICAL LIBRARY	5
TECHNICAL PUBLICATIONS & EDITING UNIT	2
DIRECTOR, OPERATIONS DIRECTORATE	1
DIRECTOR, PROCUREMENT DIRECTORATE	1
DIRECTOR, PRODUCT ASSURANCE DIRECTORATE	1

NOTE: PLEASE NOTIFY DIRECTOR, BENET WEAPONS LABORATORY, ATTN:  
DRDAR-LCB-TL, OF ANY REQUIRED CHANGES.



# EXTERNAL DISTRIBUTION LIST (CONT)

	<u>NO. OF COPIES</u>		<u>NO. OF COPIES</u>
COMMANDER US ARMY RESEARCH OFFICE P.O. BOX 12211 RESEARCH TRIANGLE PARK, NC 27709	1	COMMANDER DEFENSE DOCU CEN ATTN: DDC-TCA CAMERON STATION ALEXANDRIA, VA 22314	12
COMMANDER US ARMY HARRY DIAMOND LAB ATTN: TECH LIB 2800 POWDER MILL ROAD ADELPHIA, MD 20783	1	METALS & CERAMICS INFO CEN BATTELLE COLUMBUS LAB 505 KING AVE COLUMBUS, OHIO 43201	1
DIRECTOR US ARMY INDUSTRIAL BASE ENG ACT ATTN: DRXPE-MT ROCK ISLAND, IL 61201	1	MPDC 13919 W. BAY SHORE DR. TRAVERSE CITY, MI 49684	1
CHIEF, MATERIALS BRANCH US ARMY R&S GROUP, EUR BOX 65, FPO N.Y. 09510	1	MATERIEL SYSTEMS ANALYSIS ACTV ATTN: DRXSY-MP ABERDEEN PROVING GROUND MARYLAND 21005	1
COMMANDER NAVAL SURFACE WEAPONS CEN ATTN: CHIEF, MAT SCIENCE DIV DAHLGREN, VA 22448	1		
DIRECTOR US NAVAL RESEARCH LAB ATTN: DIR, MECH DIV CODE 26-27 (DOC LIB) WASHINGTON, D.C. 20375	1 1		
NASA SCIENTIFIC & TECH INFO FAC P.O. BOX 8757, ATTN: ACQ BR BALTIMORE/WASHINGTON INTL AIRPORT MARYLAND 21240	1		

NOTE: PLEASE NOTIFY COMMANDER, ARRADCOM, ATTN: BENET WEAPONS LABORATORY, DRDAR-LCB-TL, WATERVLIET ARSENAL, WATERVLIET, N.Y. 12189, OF ANY REQUIRED CHANGES.

# EXTERNAL DISTRIBUTION LIST

	<u>NO. OF COPIES</u>		<u>NO. OF COPIES</u>
ASST SEC OF THE ARMY RESEARCH & DEVELOPMENT ATTN: DEP FOR SCI & TECH THE PENTAGON WASHINGTON, D.C. 20315	1	COMMANDER US ARMY TANK-AUTMV R&D COMD ATTN: TECH LIB - DRDTA-UL MAT LAB - DRDTA-RK WARREN, MICHIGAN 48090	1 1
COMMANDER US ARMY MAT DEV & READ. COMD ATTN: DRCDE 5001 EISENHOWER AVE ALEXANDRIA, VA 22333	1	COMMANDER US MILITARY ACADEMY ATTN: CHMN, MECH ENGR DEPT WEST POINT, NY 10996	1
COMMANDER US ARMY ARRADCOM ATTN: DRDAR-TSS DRDAR-LCA (PLASTICS TECH EVAL CEN)	2 1	COMMANDER REDSTONE ARSENAL ATTN: DRSMI-RB DRSMI-RRS DRSMI-RSM ALABAMA 35809	2 1 1
DOVER, NJ 07801			
COMMANDER US ARMY ARRCOM ATTN: DRSAR-LEP-L ROCK ISLAND ARSENAL ROCK ISLAND, IL 61299	1	COMMANDER ROCK ISLAND ARSENAL ATTN: SARRI-ENM (MAT SCI DIV) ROCK ISLAND, IL 61202	1
DIRECTOR US Army Ballistic Research Laboratory ATTN: DRDAR-TSB-S (STINFO) ABERDEEN PROVING GROUND, MD 21005	1	COMMANDER HQ, US ARMY AVN SCH ATTN: OFC OF THE LIBRARIAN FT RUCKER, ALABAMA 36362	1
COMMANDER US ARMY ELECTRONICS COMD ATTN: TECH LIB FT MONMOUTH, NJ 07703	1	COMMANDER US ARMY FGN SCIENCE & TECH CEN ATTN: DRXST-SD 220 7TH STREET, N.E. CHARLOTTESVILLE, VA 22901	1
COMMANDER US ARMY MOBILITY EQUIP R&D COMD ATTN: TECH LIB FT BELVOIR, VA 22060	1	COMMANDER US ARMY MATERIALS & MECHANICS RESEARCH CENTER ATTN: TECH LIB - DRXMR-PL WATERTOWN, MASS 02172	2

NOTE: PLEASE NOTIFY COMMANDER, ARRADCOM, ATTN: BENET WEAPONS LABORATORY,  
DRDAR-LCB-TL, WATERVLIET ARSENAL, WATERVLIET, N.Y. 12189, OF ANY  
REQUIRED CHANGES.